


Figure 1



RECEIVED
OCT 11 1999
NIST

O I P E J C A I
AUG 18 2003
PATENT & TRADEMARK OFFICE

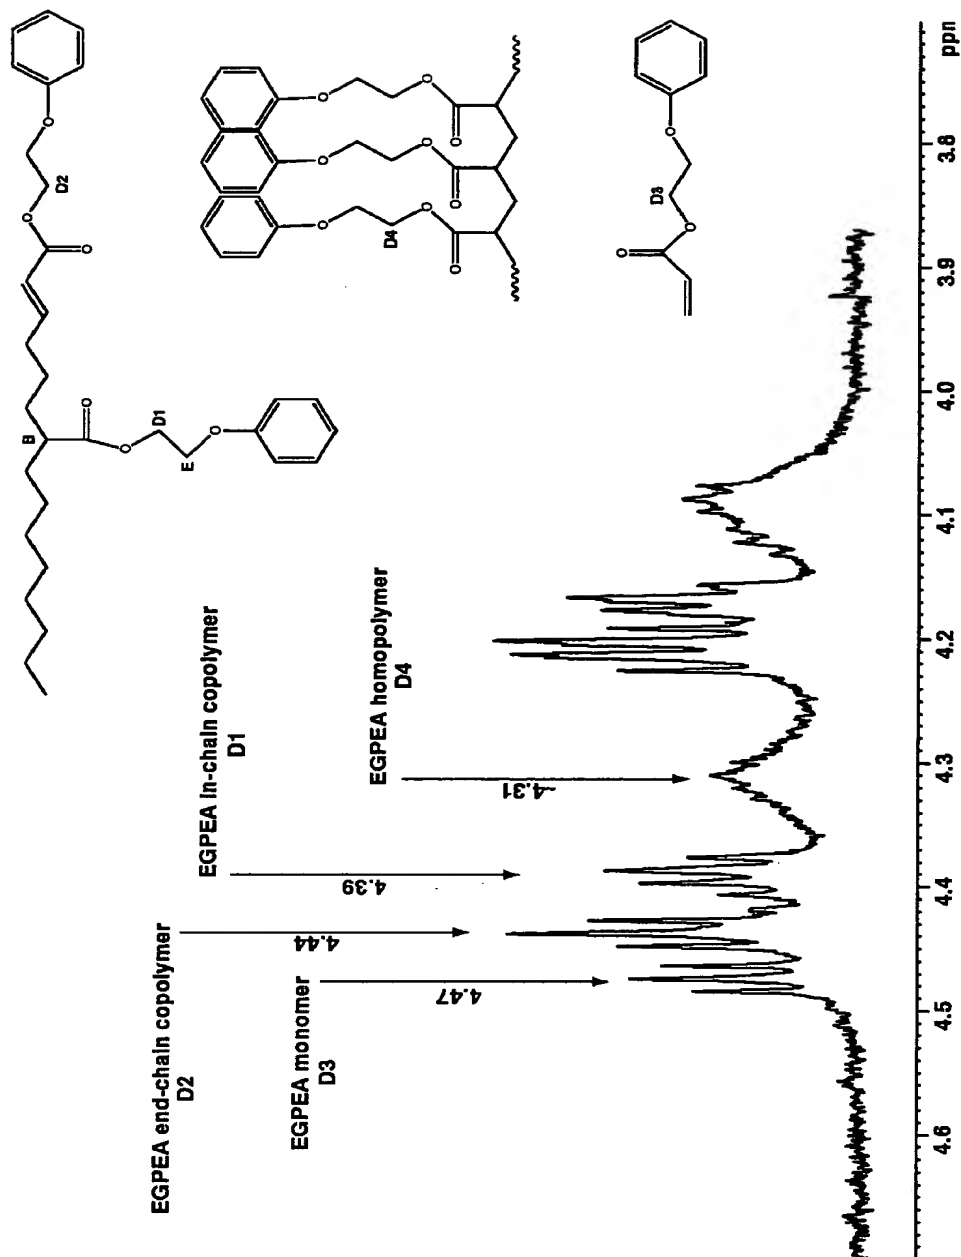

REVIEWED
2005 01 06
JMS

310mg sample and 80 mg CrAcAc in total vol 3.1 ml TCB
Varian Unity 400 NMR Spectrometer
gea4 10mm probe, 120C, a locked, 13C NMR
DuPont NMR Lab E302/118

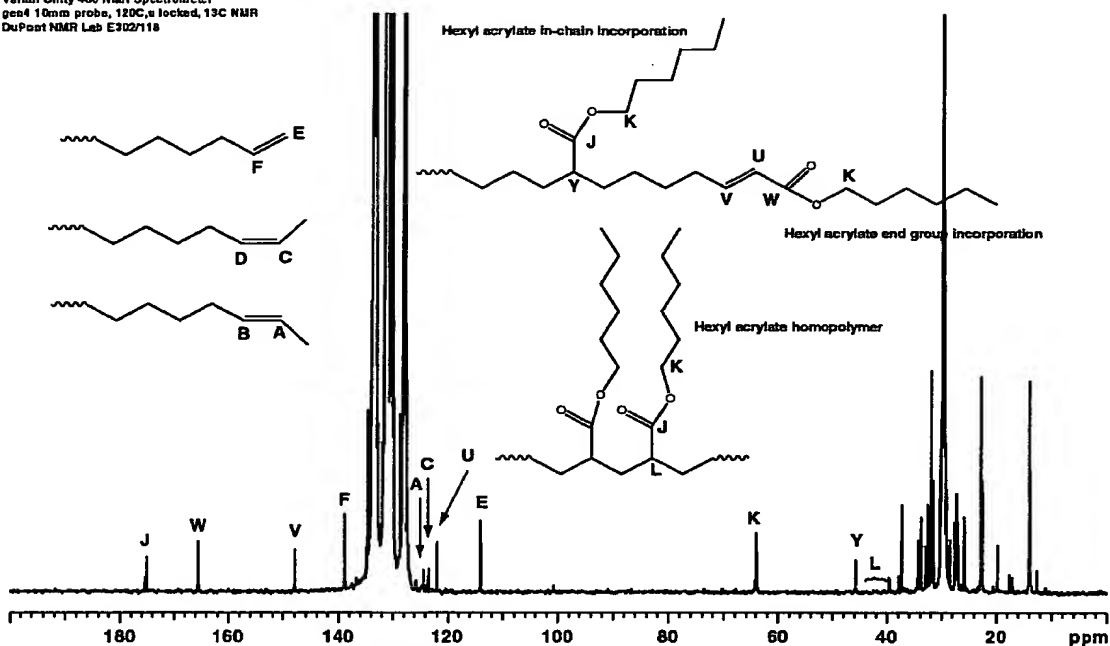


Figure 2

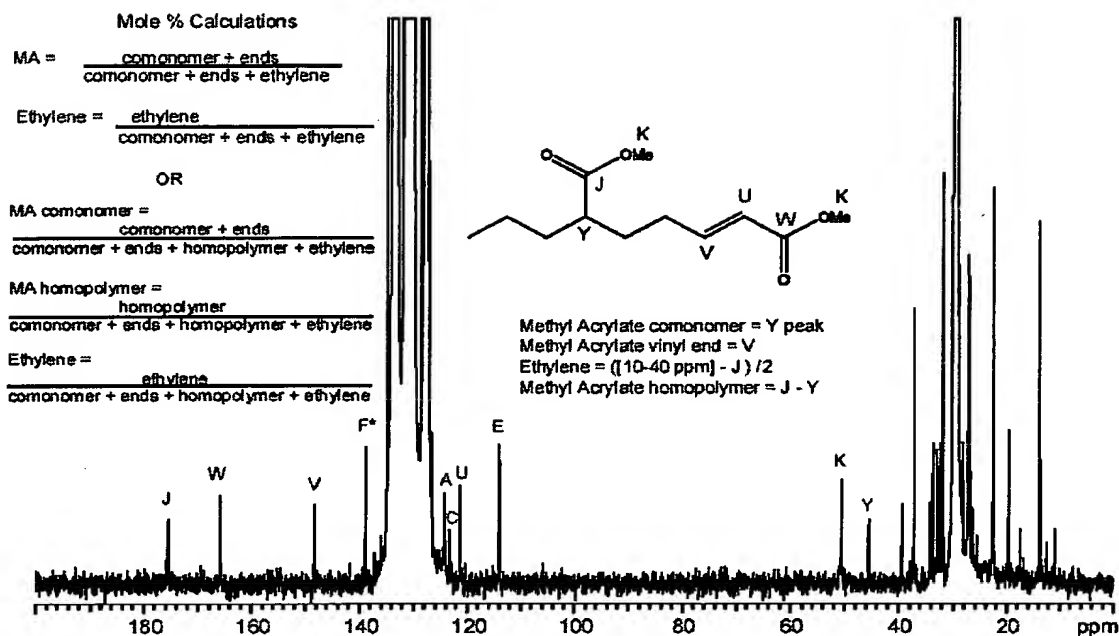


Figure 3